

本试剂盒只能用于科学研究，不得用于医学诊断

牛 (Bovine) 活性氧簇 (ROS) ELISA 检测试剂盒

使用说明书

检测原理

试剂盒采用双抗体一步夹心法酶联免疫吸附试验 (ELISA)。预先包被活性氧簇 (ROS) 抗体的包被微孔中，依次加入标本、标准品、HRP 标记的检测抗体，经过温育并彻底洗涤。用底物 TMB 显色，TMB 在过氧化物酶的催化下转化成蓝色，并在酸的作用下转化成最终的黄色。颜色的深浅和样品中的活性氧簇 (ROS) 呈正相关。用酶标仪在 450nm 波长下测定吸光度 (OD 值)，计算样品活性。

样品收集、处理及保存方法

1. 血清：使用不含热原和内毒素的试管，操作过程中避免任何细胞刺激，收集血液后，3000 转离心 10 分钟将血清和红细胞迅速小心地

分离。

2. 血浆：EDTA、柠檬酸盐或肝素抗凝。3000 转离心 30 分钟取上清。
3. 细胞上清液：3000 转离心 10 分钟去除颗粒和聚合物。
4. 组织匀浆：将组织加入适量生理盐水捣碎。3000 转离心 10 分钟取上清。
5. 保存：如果样本收集后不及时检测，请按一次用量分装，冻存于 -20°C ，避免反复冻融，在室温下解冻并确保样品均匀地充分解冻。

自备物品

1. 酶标仪 (450nm)
2. 高精度加样器及枪头：0.5-10uL、2-20uL、20-200uL、200-1000uL
3. 37°C 恒温箱

操作注意事项

1. 试剂盒保存在 $2-8^{\circ}\text{C}$ ，使用前室温平衡 20 分钟。从冰箱取出的

浓缩洗涤液会有结晶，这属于正常现象，水浴加热使结晶完全溶解后再使用。

2. 实验中不用的板条应立即放回自封袋中，密封(低温干燥)保存。
3. 浓度为 0 的 S0 号标准品即可视为阴性对照或者空白；按照说明书操作时样本已经稀释 5 倍，最终结果乘以 5 才是样本实际浓度。
4. 严格按照说明书中标明的时间、加液量及顺序进行温育操作。
5. 所有液体组分使用前充分摇匀。

试剂盒组成

名称	96 孔配置	48 孔配置	备注
微孔酶标板	12 孔×8 条	12 孔×4 条	无
标准品	0.3mL*6 管	0.3mL*6 管	无
样本稀释液	6mL	3mL	无
检测抗体-HRP	10mL	5mL	无
20×洗涤缓冲液	25mL	15mL	按说明书进行稀释
底物 A	6mL	3mL	无
底物 B	6mL	3mL	无
终止液	6mL	3mL	无

封板膜	2 张	2 张	无
说明书	1 份	1 份	无
自封袋	1 个	1 个	无

注：标准品 (S0-S5) 浓度依次为：0、30、60、120、240、480 U/ml

试剂的准备

20×洗涤缓冲液的稀释：蒸馏水按 1：20 稀释，即 1 份的 20×洗涤缓冲液加 19 份的蒸馏水。

洗板方法

1. 手工洗板：甩尽孔内液体，每孔加满洗涤液，静置 1min 后甩尽孔内液体，在吸水纸上拍干，如此洗板 5 次。
2. 自动洗板机：每孔注入洗液 350 μL，浸泡 1min，洗板 5 次。

操作步骤


1. 从室温平衡 20min 后的铝箔袋中取出所需板条，剩余板条用自封袋密封放回 4℃。
2. 设置标准品孔和样本孔，标准品孔各加不同浓度的标准品 50 μL；

3. 样本孔先加待测样本 10 μ L，再加样本稀释液 40 μ L；空白孔不加。
4. 除空白孔外，标准品孔和样本孔中每孔加入辣根过氧化物酶（HRP）标记的检测抗体 100 μ L，用封板膜封住反应孔，37 $^{\circ}$ C 水浴锅或恒温箱温育 60min。
5. 弃去液体，吸水纸上拍干，每孔加满洗涤液，静置 1min，甩去洗涤液，吸水纸上拍干，如此重复洗板 5 次（也可用洗板机洗板）。
6. 每孔加入底物 A、B 各 50 μ L，37 $^{\circ}$ C 避光孵育 15min。
7. 每孔加入终止液 50 μ L，15min 内，在 450nm 波长处测定各孔的 OD 值。

结果判断

绘制标准曲线：在 Excel 工作表中，以标准品浓度作横坐标，对应 OD 值作纵坐标，绘制出标准品线性回归曲线，按曲线方程计算各样

本浓度值。

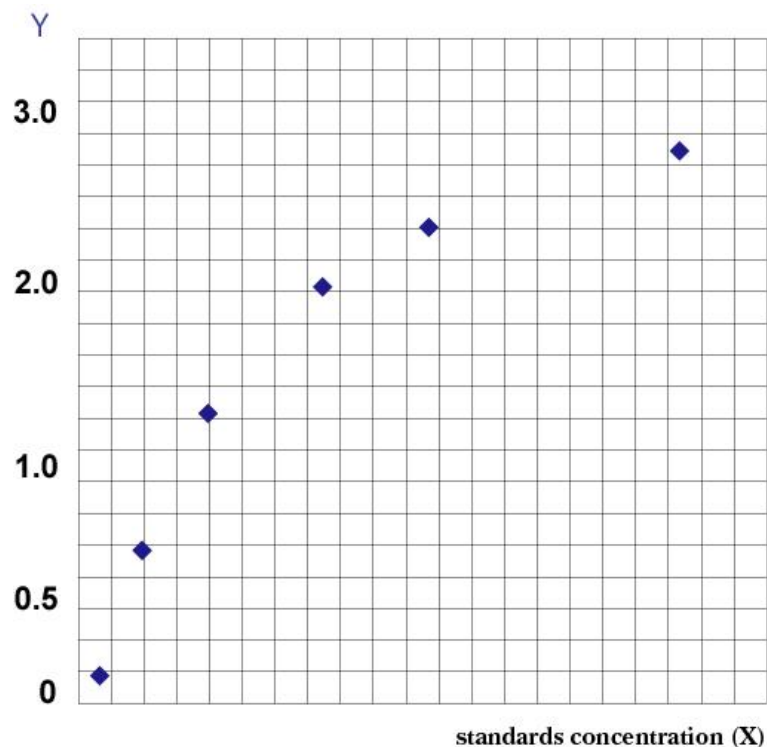

试剂盒性能

1. 准确性：标准品线性回归与预期浓度相关系数 R 值，大于等于 0.9900。

2. 灵敏度：最低检测浓度小于 1.0 U/ml。
3. 特异性：不与其它可溶性结构类似物交叉反应。
4. 重复性：板内、板间变异系数均小于 15%。
5. 贮藏：2-8℃，避光防潮保存。
6. 有效期：6 个月

免责声明

1. 试剂盒仅供研究使用，不得用于临床实验或人体实验，否则所产生的一切后果，由实验者承担，本公司概不负责。
2. 严格按照说明书操作，实验者违反说明书操作，后果由实验者承担。

**FOR RESEARCH USE ONLY.
NOT FOR USE IN DIAGNOSTIC PROCEDURES.**

Bovine reactive oxygen species (ROS) ELISA Kit instruction

Intended use

This ROS ELISA kit is intended Laboratory for Research use only and is not for use in diagnostic or therapeutic procedures. The Stop Solution changes the color from blue to yellow and the intensity of the color is measured at 450 nm using a spectrophotometer. In order to measure the concentration of ROS in the sample, this ROS ELISA Kit includes a set of calibration standards. The calibration standards are assayed at the same time as the samples and allow the operator to produce a standard curve of Optical Density versus ROS concentration. The concentration of ROS in the samples is then determined by comparing the O.D. of the samples to the standard curve.

Sample collection and storages

Serum - Use a serum separator tube and allow samples to clot for 30 minutes before centrifugation for 10 minutes at approximately 3000×g. Remove serum and

assay immediately or aliquot and store samples at -20°C or -80°C. Avoid repeated freeze-thaw cycles

Plasma - Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge samples for 30 minutes at 3000×g at 2-8°C within 30 minutes of collection. Store samples at -20°C or -80°C. Avoid repeated freeze-thaw cycles.

Cell culture supernates and other biological fluids - Remove particulates by centrifugation and assay immediately or aliquot and store samples at -20°C or -80°C. Avoid repeated freeze-thaw cycles.



Note: The samples should be centrifuged adequately and no hemolysis or granule was allowed.

Materials required but not supplied

1. Standard microplate reader(450nm)
2. Precision pipettes and Disposable pipette tips.
3. 37 °C incubator

Precautions

1. Do not substitute reagents from one kit to another. Standard, conjugate and microplates are matched for optimal performance. Use only the reagents supplied by

manufacturer.

2. Do not remove microplate from the storage bag until needed. Unused strips should be stored at 2-8°C in their pouch with the desiccant provided.
3. Mix all reagents before using.

Remove all kit reagents from refrigerator and allow them to reach room temperature (20-25°C)

Materials supplied

Name	96 determinations	48 determinations
Microelisa stripplate	12*8strips	12*4strips
Standard	0.3ml*6tubes	0.3ml*6tubes
Sample Diluent	6.0ml	3.0ml
HRP-Conjugate reagent	10.0ml	5.0ml
20X Wash solution	25ml	15ml
Chromogen Solution A	6.0ml	3.0ml
Chromogen Solution B	6.0ml	3.0ml
Stop Solution	6.0ml	3.0ml
Closure plate membrane	2	2
User manual	1	1
Sealed bags	1	1

Note: Standard (S0 → S5) concentration was followed by:0,30,60,120,240,480 U/ml

Reagent preparation

20×wash solution:Dilute with Distilled or deionized water 1:20.

Assay procedure

1. Prepare all reagents before starting assay procedure. It is recommended that all Standards and Samples be added in duplicate to the Microelisa Stripplate.
2. Add standard: Set Standard wells, testing sample wells. Add standard 50μl to standard well.
3. Add Sample: Add testing sample 10μl then add Sample Diluent 40μl to testing sample well; Blank well doesn't add anything.
4. Add 100μl of HRP-conjugate reagent to each well, cover with an adhesive strip and incubate for 60 minutes at 37°C.
5. Aspirate each well and wash, repeating the process four times for a total of five washes. Wash by filling each well with Wash Solution (400μl) using a squirt bottle, manifold dispenser or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Solution by aspirating or decanting. Invert the plate and blot it against clean paper towels.


6. Add chromogen solution A 50μl and chromogen solution B 50μl to each well. Gently mix and incubate for 15 minutes at 37°C. **Protect from light.**
7. Add 50μl Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green or the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
8. Read the Optical Density (O.D.) at 450 nm using a microtiter plate reader within 15 minutes.

Calculation of results

1. This standard curve is used to determine the amount in an unknown sample. The standard curve is generated by plotting the average O.D. (450 nm) obtained for each of the six standard concentrations on the vertical (Y) axis versus the corresponding concentration on the horizontal (X) axis.
2. First, calculate the mean O.D. value for each standard and sample. All O.D. values, are subtracted by the mean value of the zero standard before result interpretation. Construct the standard curve using graph paper or statistical software.
3. To determine the amount in each sample, first locate the O.D. value on the Y-axis and extend a horizontal line to the standard curve. At the point of

intersection, draw a vertical line to the X-axis and read the corresponding concentration.

- Any variation in operator, pipetting and washing technique, incubation time or temperature, and kit age can cause variation in result. Each user should obtain their own standard curve.
- The sensitivity by this assay is 1.0 U/ml
- Standard curve

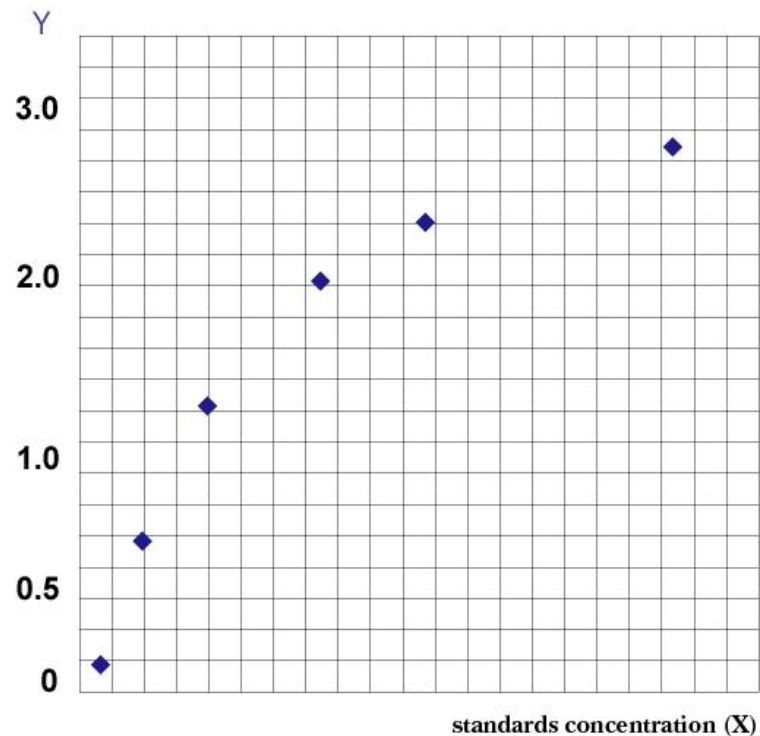

Storage: 2-8°C.

validity: six months.

**FOR RESEARCH USE ONLY; NOT FOR THERAPEUTIC OR
DIAGNOSTIC APPLICATIONS! PLEASE READ THROUGH
ENTIRE PROCEDURE BEFORE BEGINNING!**